


Dose to clear for varying PMMA thickness

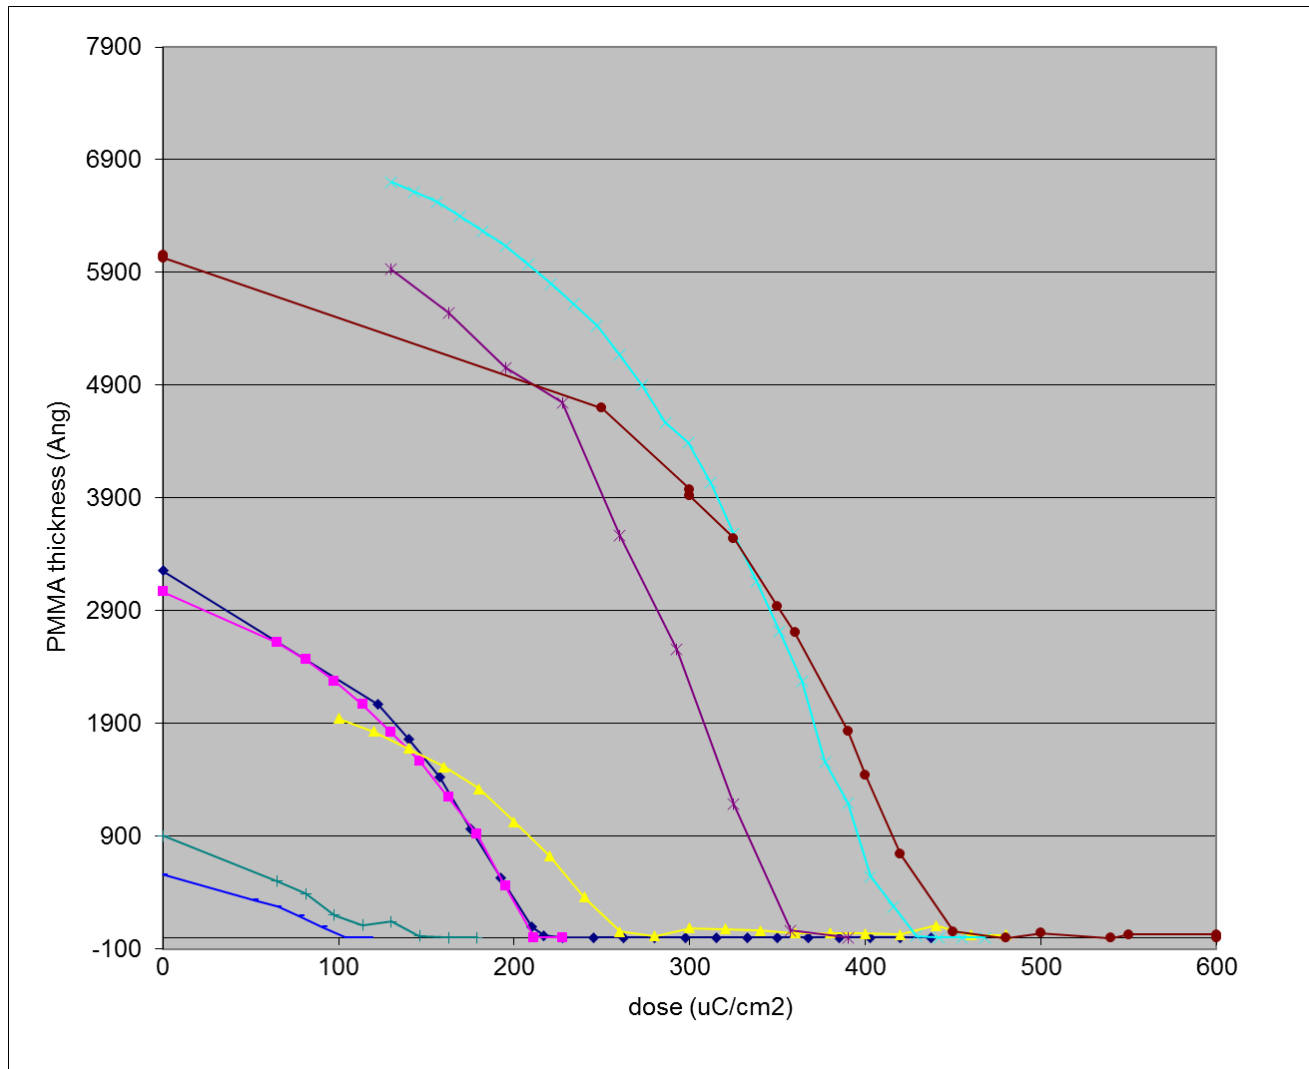

- the dose to clear increases as PMMA thickness increases
- there is some sample to sample variability in dose to clear for samples of similar thickness
- all of the samples had same develop conditions (1:1 MIBK:IPA for 2 min)